Needleless filling / Natural effect / Comfortable&painless

DESKTOP EMFACE

Instruction Manual

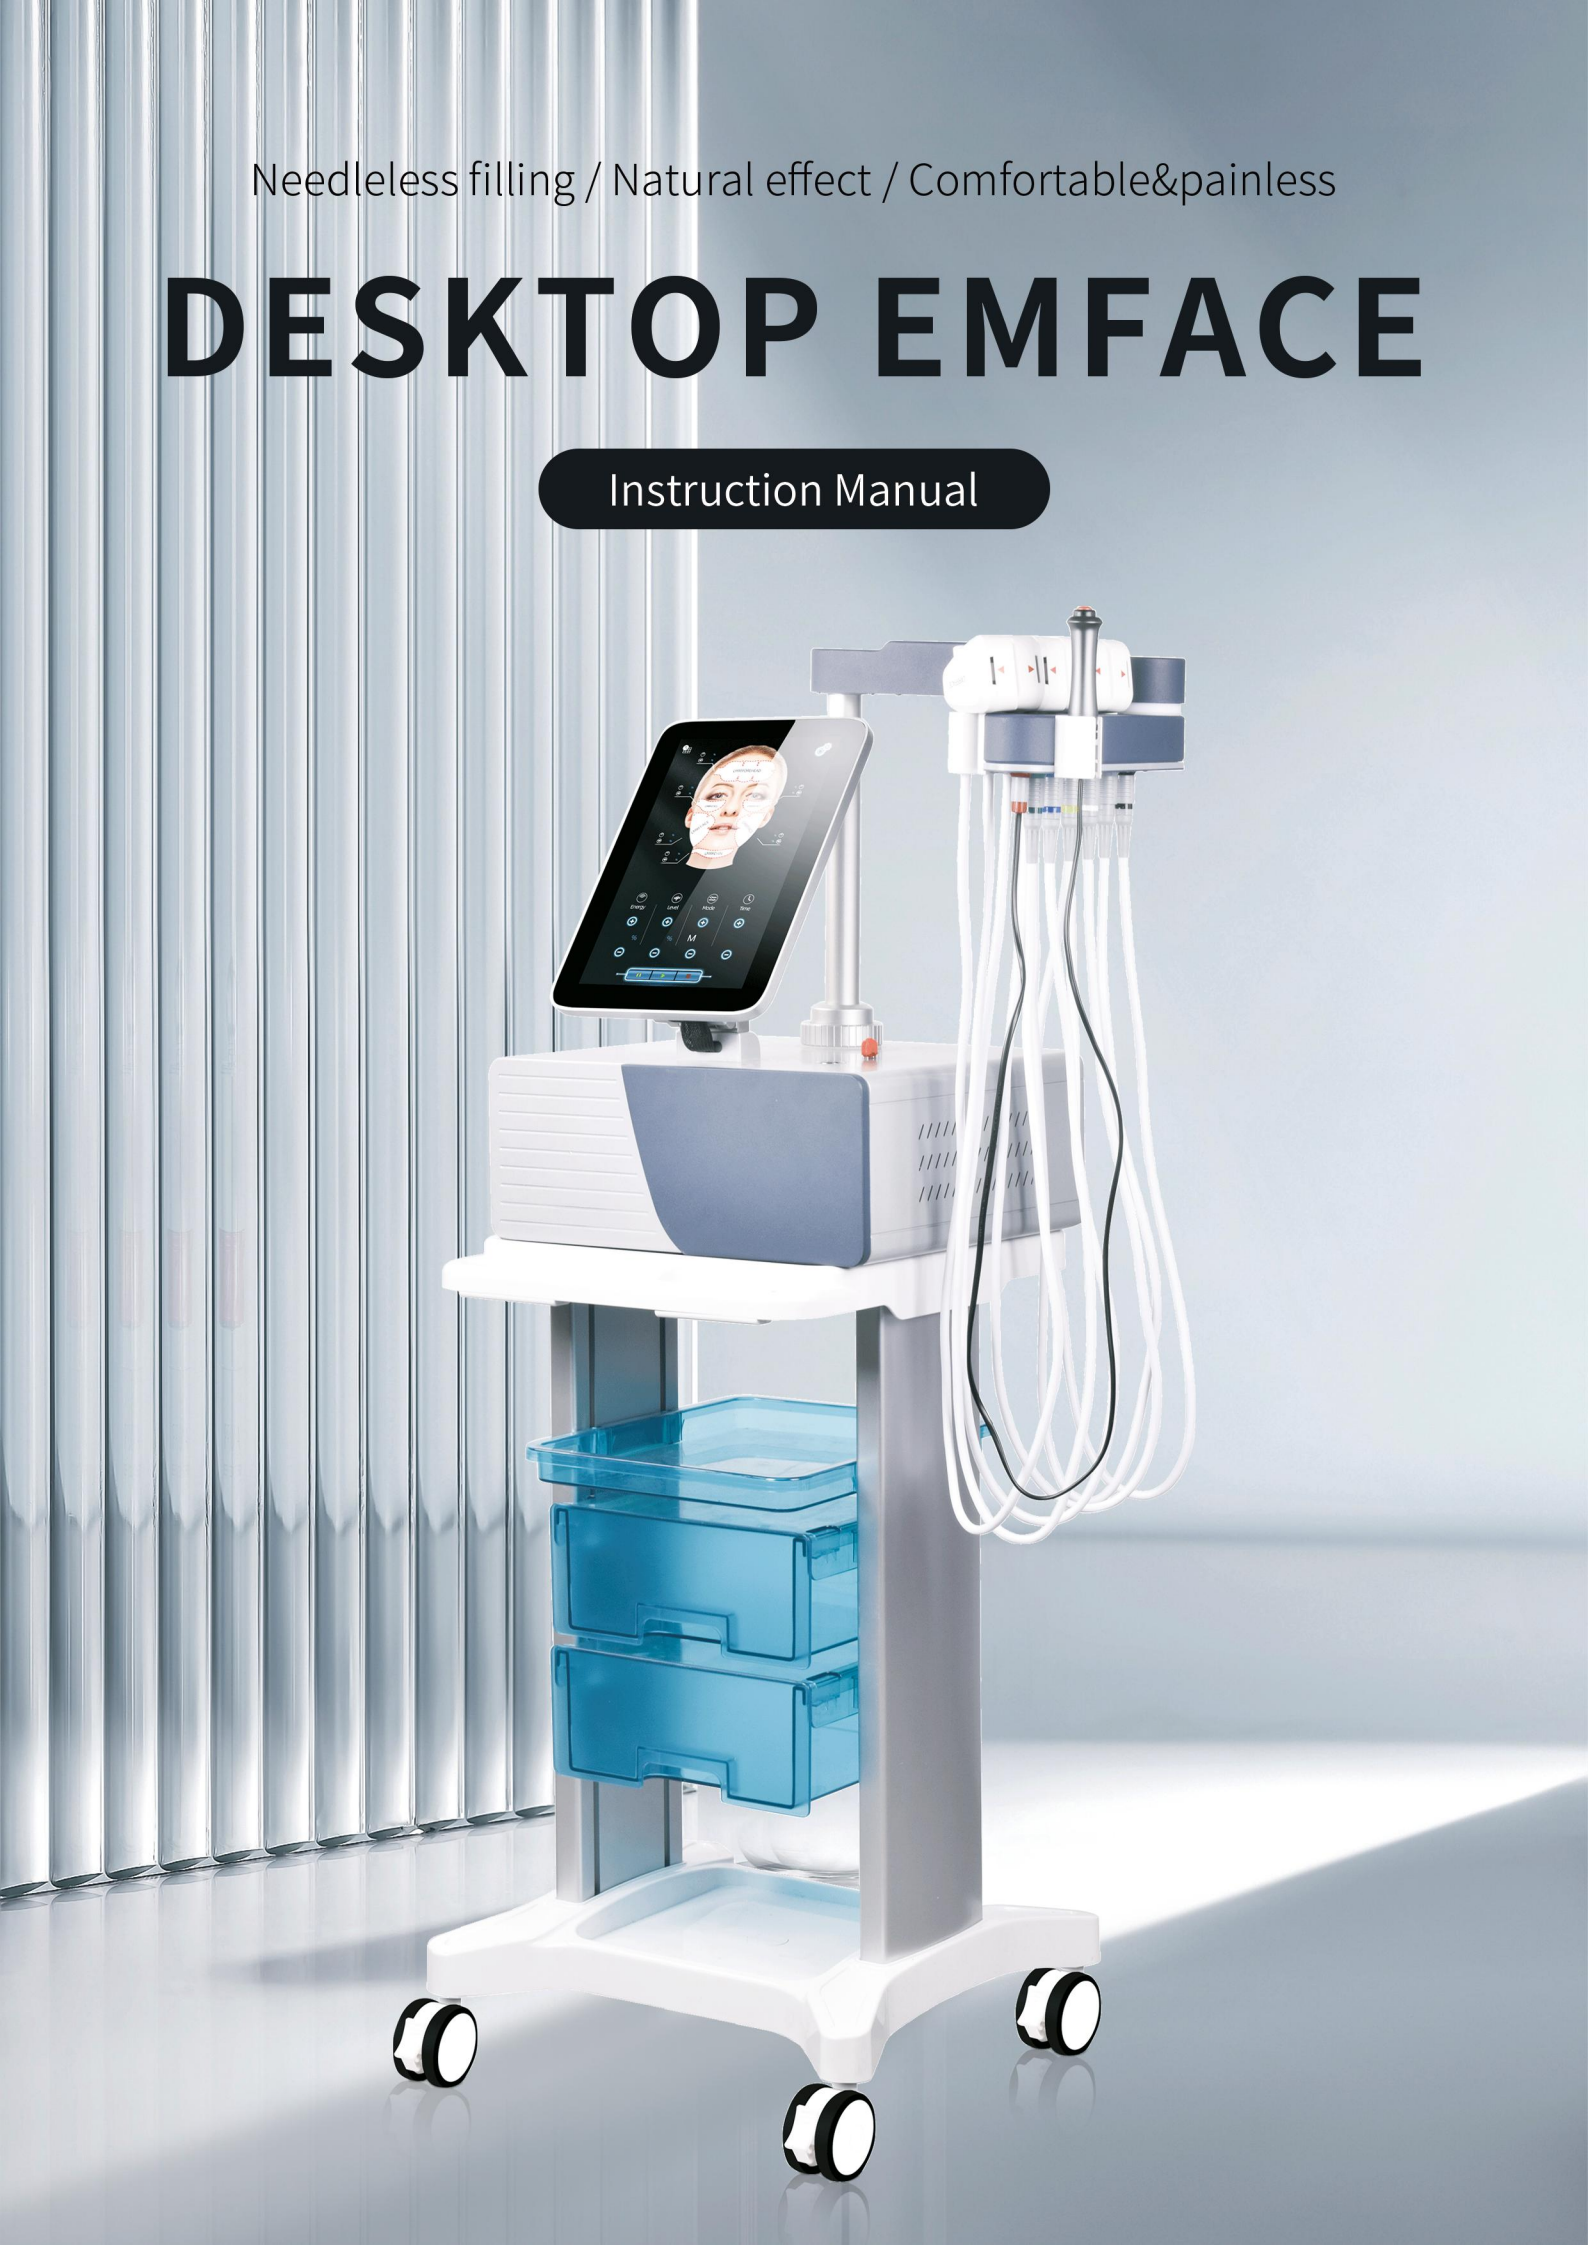

Table of Contents

Product Introduction

Working Principle 01
Product Parameter 01
Product Structure Introduction 02

Instruction for Use

Interface Introduction 04
Parameters Setting 09
Contraindications 09
Precaution 10
Accessories List 10

Product Introduction

EMFace

(EMFace) can be a muscle layer instrument, with the increase of age, the loss of muscle tissue leads to face sagging, plumpness decline, lack of facial support skin sag and other problems emface can effectively solve. Especially when the apple muscle begins to sag, emface can strengthen the facial lifting muscle group and provide deep support, and then do fascia lifting (ultrasonic knife), dermis lifting (radio frequency such as hot maggie) and dermis lifting (photoelectric project) when you can get twice the result with half the effort. If you want to fight aging sagging, you must have multiple levels of maintenance.

Working Principle

The working principle of EMFace is: one is the RF principle, and the other is the proprietary HIFES™ technology energy, also known as high intensity focused electric field, designed to stimulate facial muscles. Radiofrequency stimulates the production of collagen by heating the skin tissue, thereby improving the texture and elasticity of the skin, while the high-intensity focused electric field stimulates the deep facial muscles and collagen to achieve tissue remodeling, effectively improving the aging problem caused by the loss of facial muscle tissue.

Product Parameter

EMFace参数	
Screen size	12寸
Eye energy	10%-100%
Facial energy	10%-100%
Forehead energy	0%-100%
Body energy	10%-100%
Package size	55.5CM*46CM*53CM
Language	Various languages can be customized
Weight	26.6KG

Product Introduction

Product Structure Introduction

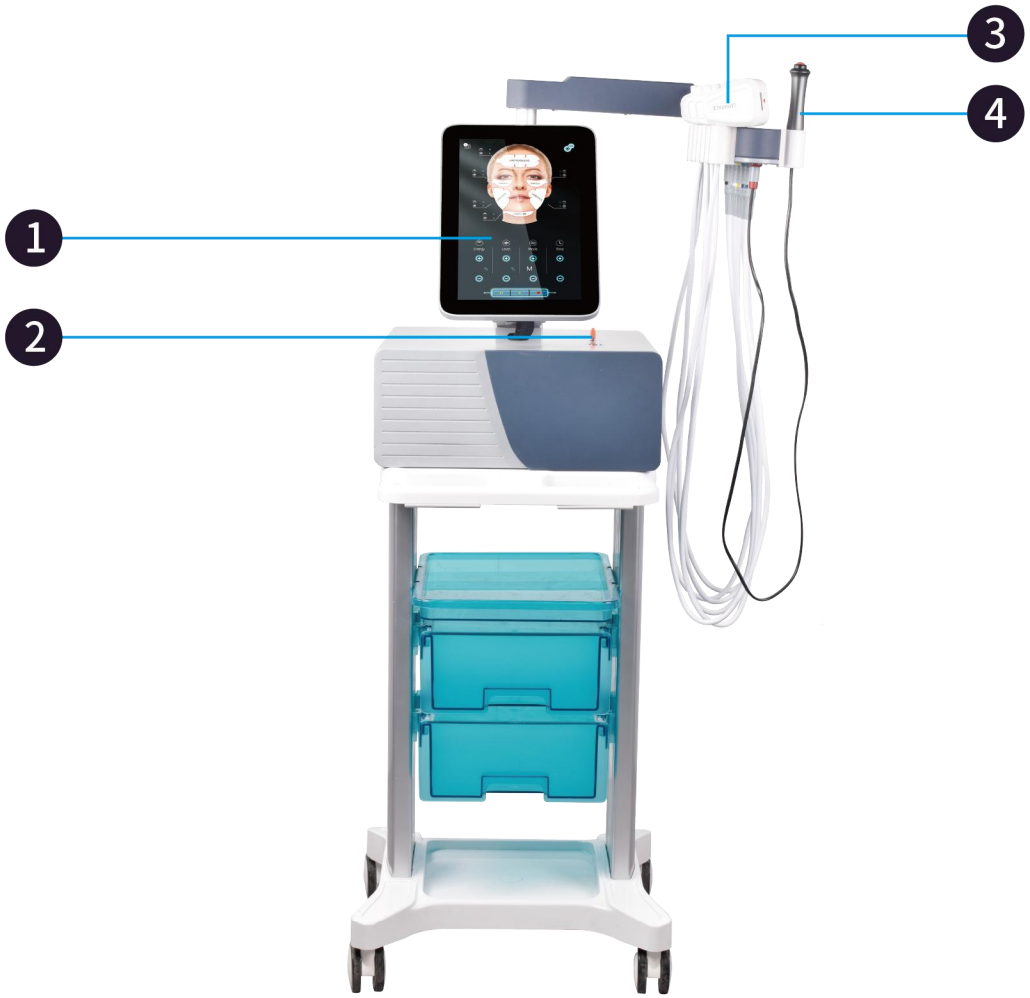

Product Front

(The picture is subject to the actual object)

1 Super Clear Touch screen 2 USB Socket

3 Adapter Box 4 Handheld Emergency Stop Stick

Product Introduction

Product Structure Introduction

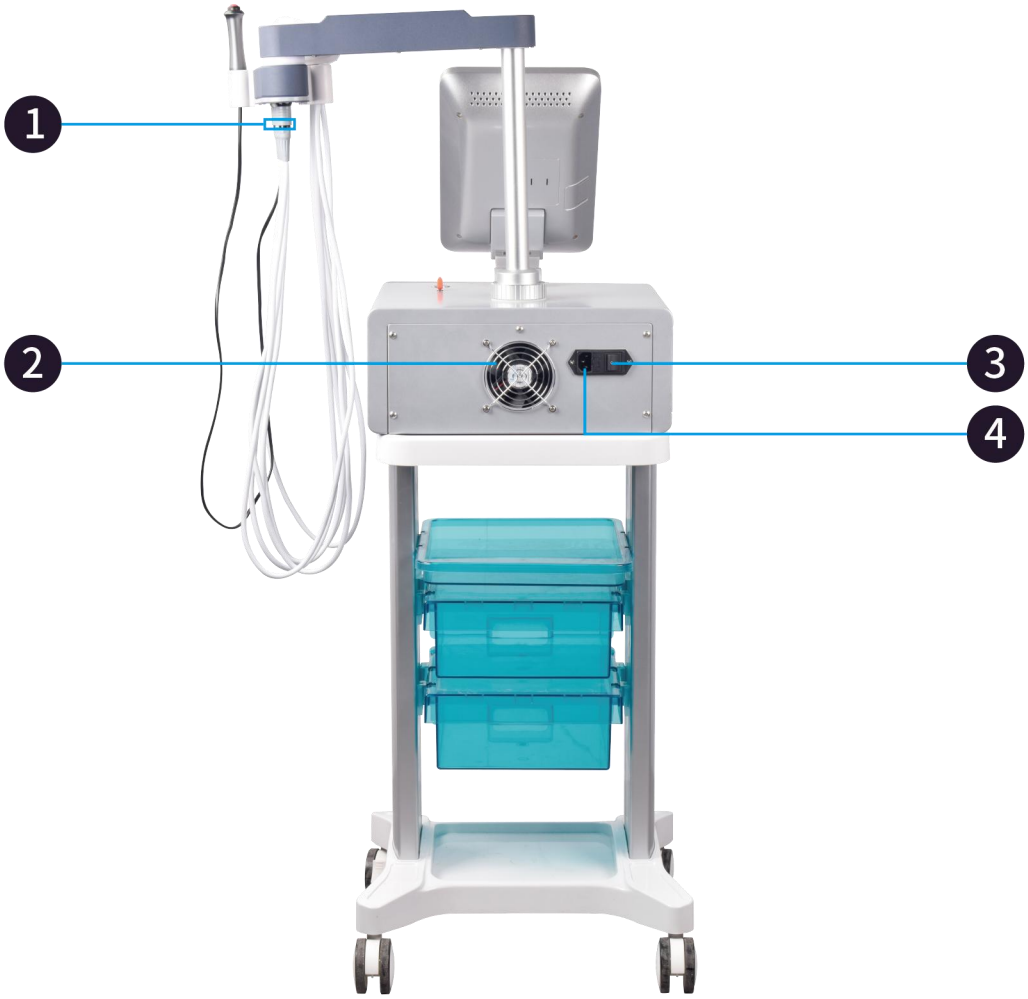

Product Back

(The picture is subject to the actual object)

1 Emergency Stop Stick Plug And A1,A2,B1,B2,C1,C2 Plug

2 Cooling fan 3 Power switch 4 Power Cable Socket

Instruction for Use

Interface Introduction

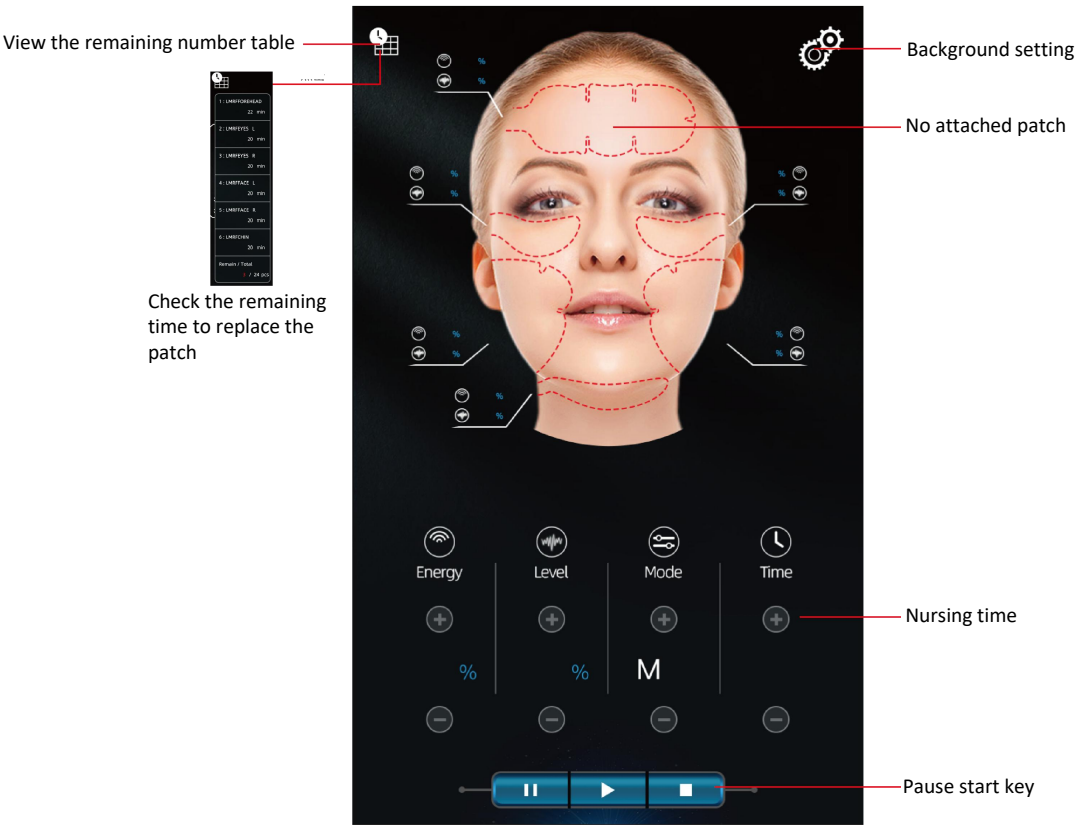

(1-1)

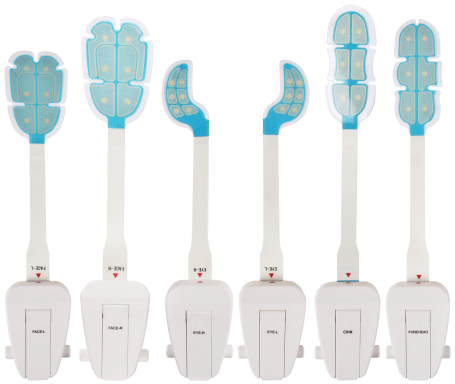

(1-2)

Before operation, connect the face USB flash drive system (black USB flash drive) to the instrument, turn on the device, and the interface shown in Figure (1-1) appears. The interface is: No patch is connected; Then connect the tiles to the converter box one by one, as shown in Figure 1-2.

Instruction for Use

Interface Introduction

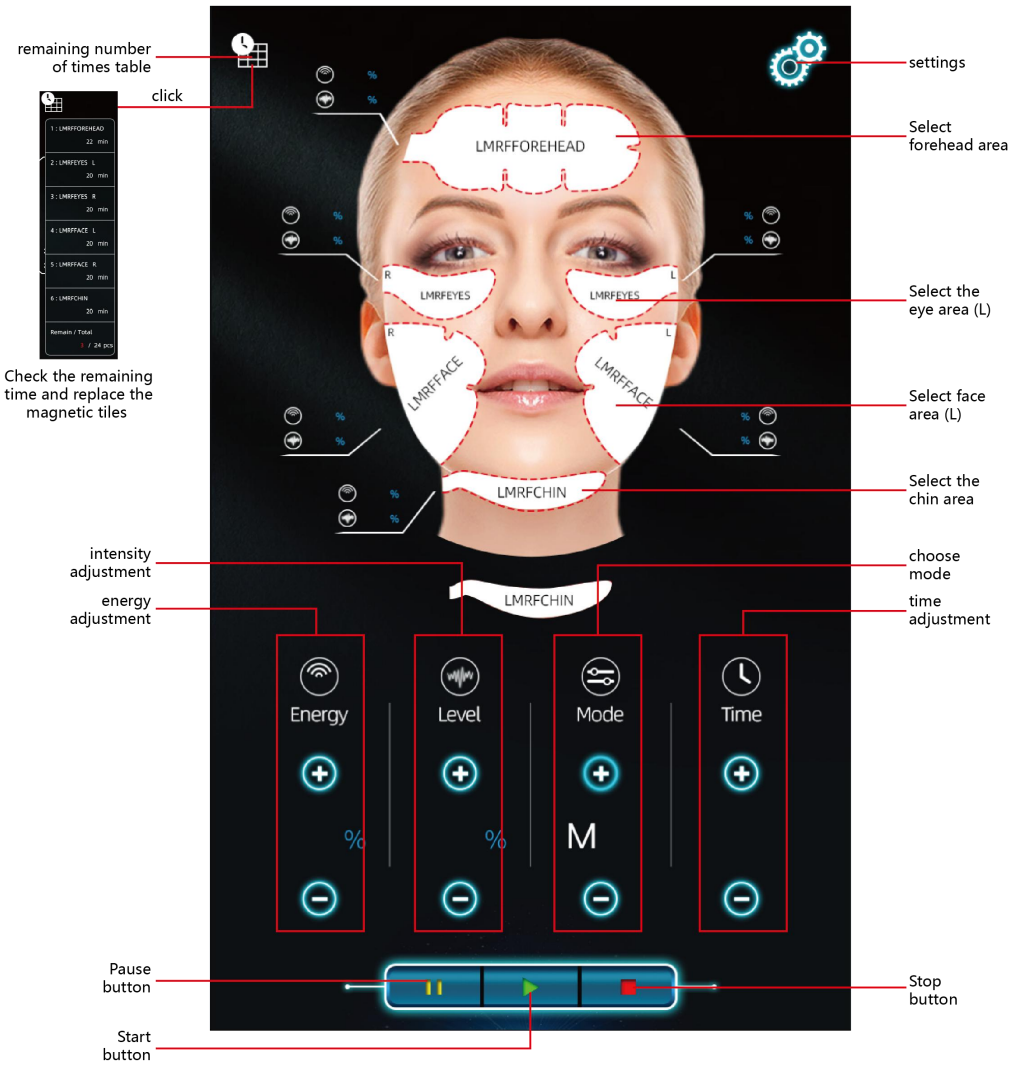

(1-3)

1, one corresponds to the connection of the magnet and the converter box, as shown in Figure (1-3). If the connection is wrong, a message will be displayed on the interface, and the connection is correct again;
2. After the magnetic patch is attached to the nursing area, adjust the energy, intensity, mode and time. At the beginning, the energy is adjusted from the lowest level, and then the energy intensity is adjusted higher after two minutes of adaptation.
3, when adjusting the energy and intensity, you need to first click the part that needs to be adjusted, and then add or reduce the energy size (such as adjusting the jaw, the interface will synchronously appear the jaw interface, and then adjust it);
4, the energy of the forehead area is smaller than the energy and intensity of other parts, and the operation time is recommended at 20 minutes.

Interface Introduction

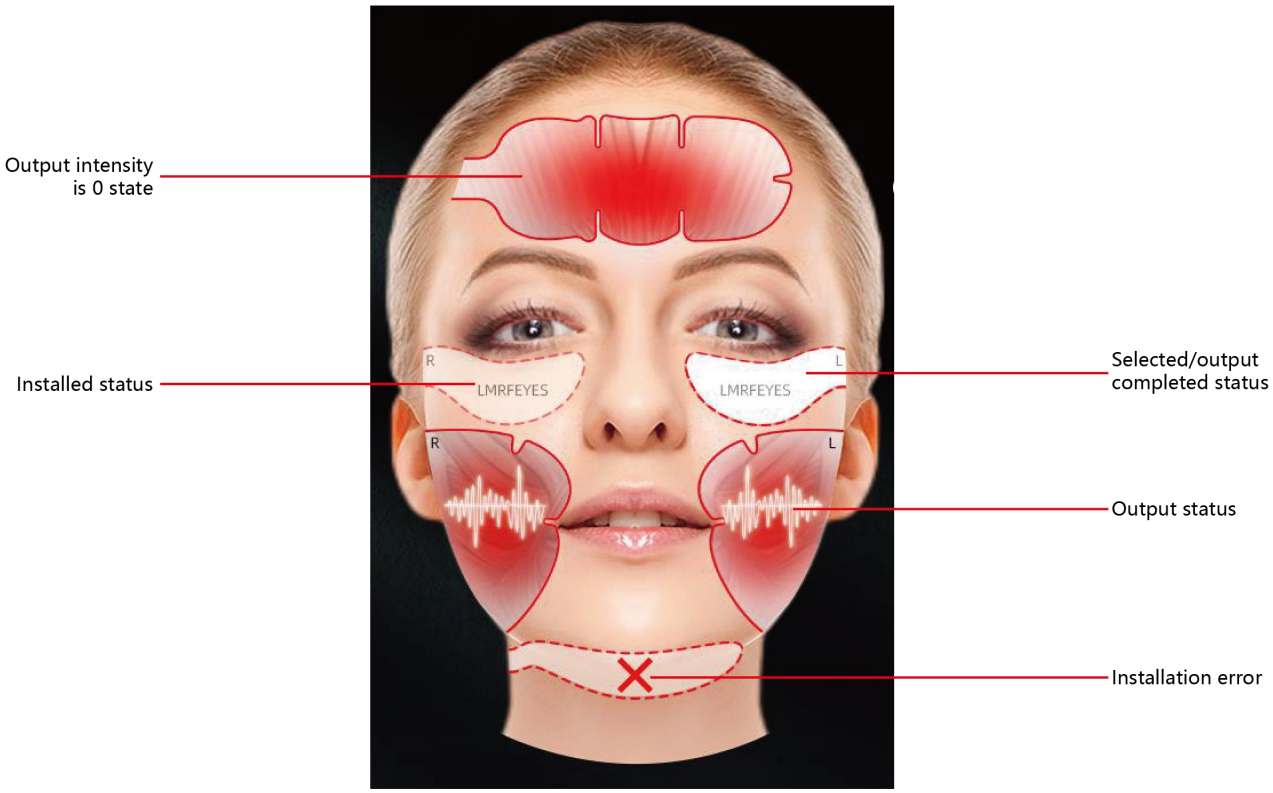

(1-4)

When the patch is applied to the face, the screen will show the part, and the instrument will stop automatically after the operation, as shown in Figure 1-4; If the installation is incorrect, the screen will prompt you to reinstall it.

Instruction for Use

Interface Introduction



(2-1)

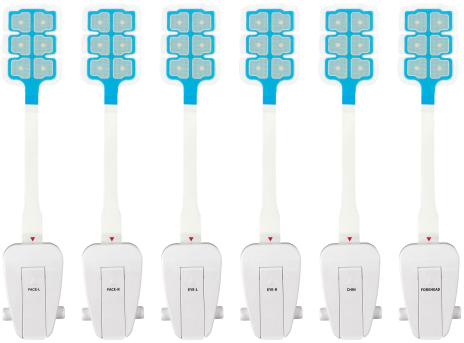

(2-2)

Figure (2-1) shows the body operation interface. Before operation, connect the body USB flash drive system (red USB flash drive) to the instrument and turn on the device. The interface shown in Figure (2-1) is: No patch is connected; Connect the patch with the conversion box. The body patch is equipped with a conversion box without distinguishing parts, as shown in Figure 2-2.

Instruction for Use

Interface Introduction

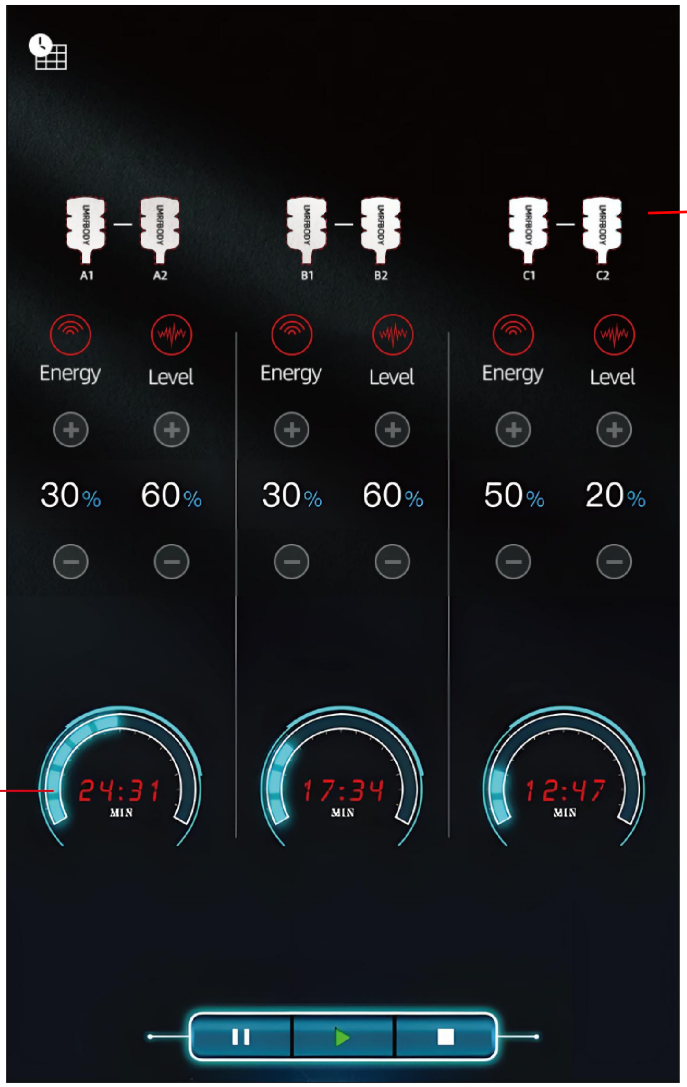

(2-3)

1, after connecting the patch and the converter box, as shown in the figure (2-3), if the connection error interface will prompt the connection error, reconnect correctly;
2, after the patch is attached to the area of care, adjust the energy, intensity, mode and time, the energy is adjusted from the lowest at the beginning, and then the energy intensity is adjusted higher after two minutes of adaptation;
3, when adjusting the energy and intensity, you need to first click the patch that needs to be adjusted, and then add or subtract the energy size.

Instruction for Use

Parameters Setting

Parameters Setting

(The actual operation situation is adjusted according to the patient's treatment)

MFace	Eye	Face	Forehead	Body
Energy	Start at 10%	Start at 40%	Start at 10%	Start at 40%
Time	20 minutes	30minutes	20 minutes	30 minutes

Contraindications

1, pregnant women, hypertension, heart disease, diabetes, hyperthyroidism patients;

2. Do not operate the instrument within three months after facial surgery;

3. People with open wounds;

4. People who have received radiation therapy for less than 3 months;

5, people with skin diseases or inflamed parts, people with suppurative acne;

6. Do not operate three hours before drinking.

7. It is prohibited to use people with more teeth.

Instruction for Use

Precaution

1. Pay attention to sun protection after operation, and take a mask every day for 3-5 consecutive days to strengthen hydration;
2, do not wash your face with hot water within 24 hours after operation, do not swim in hot springs or saunas if the water does not exceed body temperature;
3, try to avoid wearing heavy makeup immediately after operation, you can wear simple makeup;
4. During the period of skin redness after operation, it is best to avoid strong exercise and avoid sweating;
5, treatment with other instruments, at least one week apart, except for basic care;

Accessories List

Name	quantity
mainframe	1
Transfer box	6 kits
sets of face tiles	2 kits
sets of body magnets	2 kits
hand-held scram stick pendant	1
Hand-held emergency rod	1
power cable	1

Note: Be sure to inform the customer that if you feel uncomfortable during operation, press the button on the hand-held emergency stop rod immediately to stop the output of the instrument; When necessary, press the button again to output;