Mole&Freckle Removal / Pores Shrinkage/ Whitening & Rejuvenating

LIGHT SPEED PICO B

User Manual



Catalog

Product Introduction

Working Principle 01

Product Parameter 01

Product Structure Introduction 02

Instruction for use

Interface Introduction 04

Parameters Setting 06

Contraindications..... 06

Precautions 06

Matters need attention 06

product presentation

principle of the product


It has an ultra-short pulse time (as short as 375-450 picoseconds), which is faster
than the PICOSURE Honeycomb picoseconds, hence the name. Due to the fast speed, the energy peak that can be generated instantly is larger, and the pigment particles can be removed more cleanly through the "photoshock effect". At the same time, due to the ultra-short pulse width, the light energy is too late to be converted into too much heat energy, so the damage to the surrounding tissues is less, the postoperative recovery period can be greatly shortened, the side effects such as anti- black can be avoided, and the number of treatments can be reduced. In addition, its unique holographic focusing probe can amplify the energy to 22 times, and the dissolution of pigment is better.

Product parameters:

Machine power	3000W
Wave length	1064nm,532nm755nm
Facula	2-10mm
Laser output frequency	1-10Hz(adjustable)
Cooling system	Air cooling + Water cooling + Radiator

product presentation


Product structure description

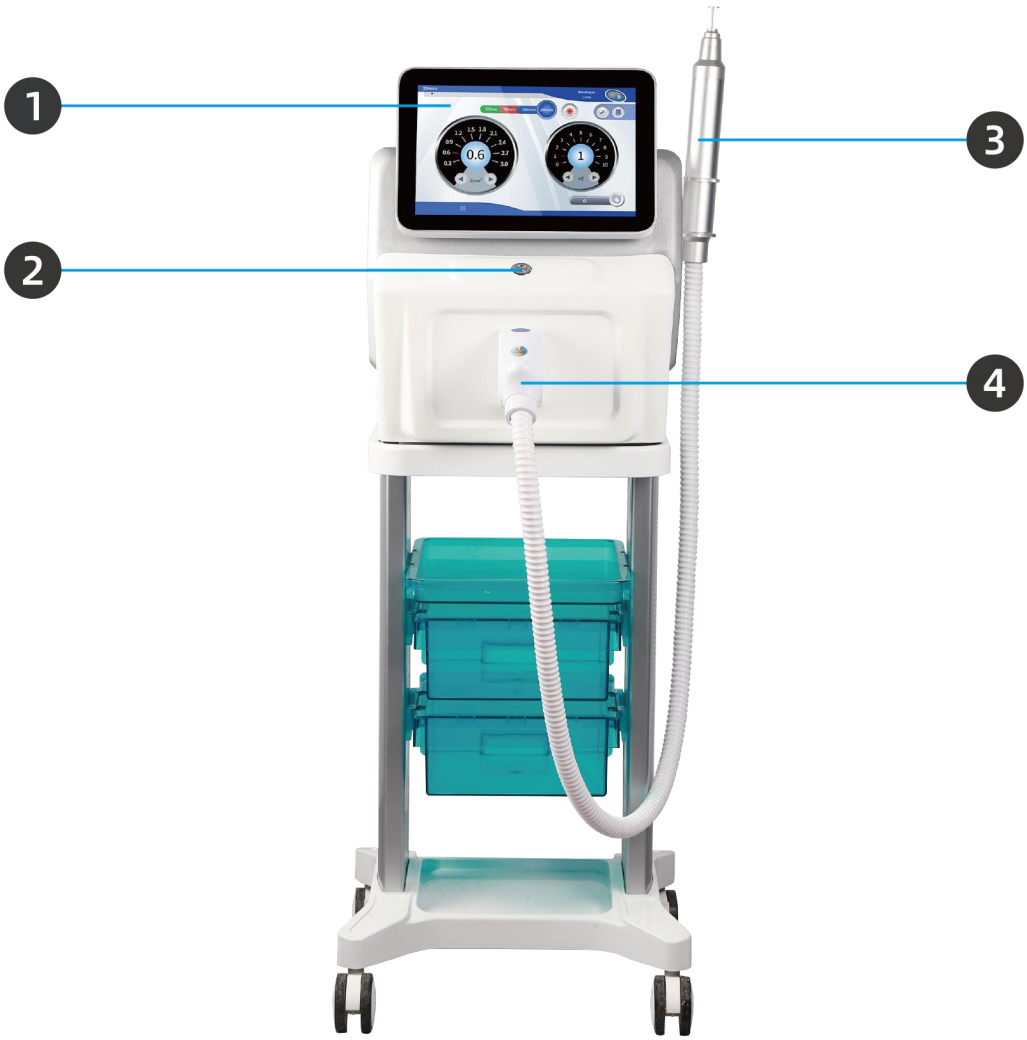

The front of machine
(Product in kind prevails)

1. 12 inch Touchable Display
2. On/off button
3. Laser handle socket
4. Laser handle

Product structure description

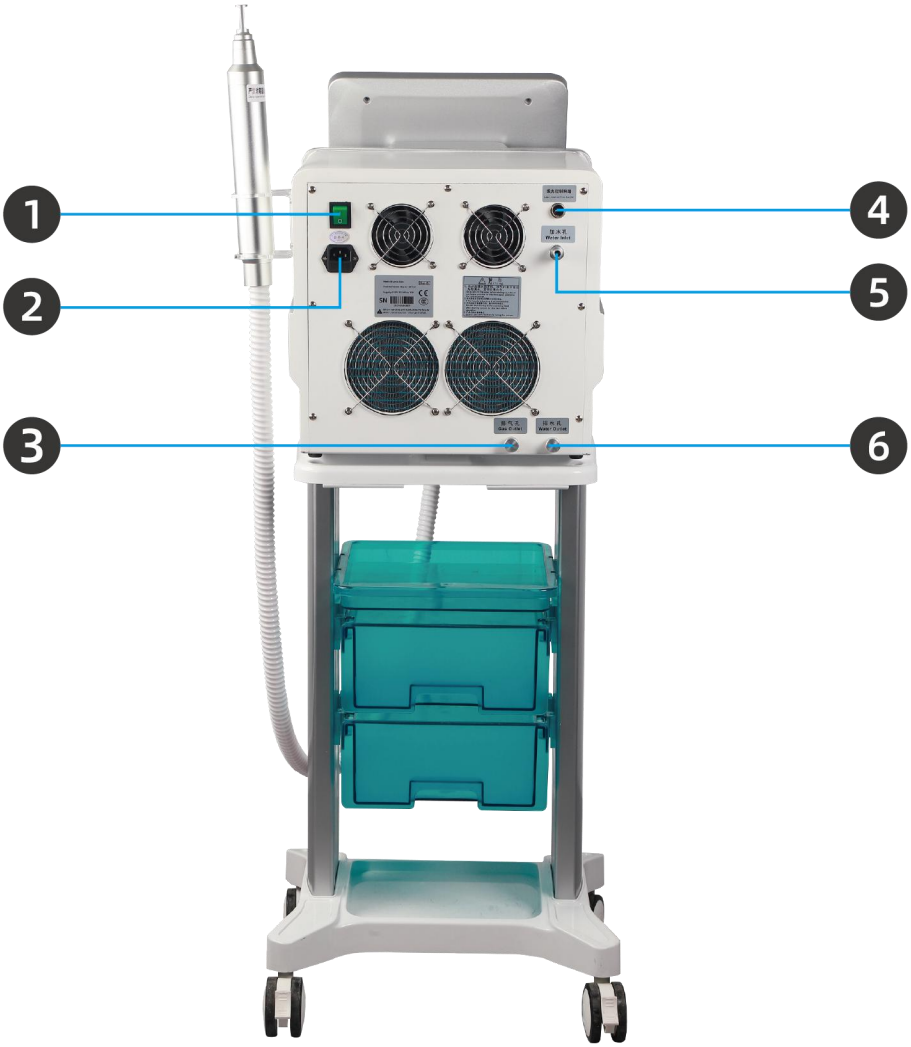


The front of machine
(Product in kind prevails)

1 Power switch
2 Power cord socket
3 Gas Outlet
4 Pedal Socket
5 Water Inlet
6 Water Outlet

Instructions

Interface description

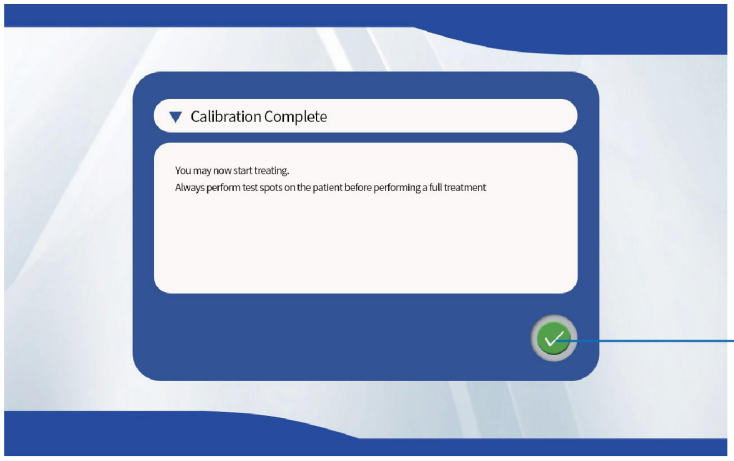

(1-1)

1-1Interface Click to enter the operation interface diagram1-2



(1-2)

Figure 1-2 shows the operation interface. Adjust the energy, frequency, wavelength, and point according to the parameter setting table Hit red aim, click standby, take out the handle, align the treatment site, step on the foot treatment began; After treatment, click standby, place the handle, and turn off the power of the instrument.

Instructions

Refer to the table for parameter Settings

The actual operation is adjusted according to the situation reflected in the patient's treatment

Type	Energy/cm²	Wave lengthnm	Remark
Brightening and anti-yellowing	0.9 1.2	1064/755	Operate until skin is reddish
Cuticular plaque	1.0-1.2	1064/755	Operate until spots turn white and bleed slightly
Chorioplaque	0.9-1.2	1064	Operate until slightly red or out of control
Chloasma	0.7 1.0	1064	Operate until pale or reddish
Mole removal	1.0-1.3	1064	Operate until blood oozes or turns white
Eyebrow tattooing, tattoos,	1.3-1.5	1064	New tattoo, black and blue, work until it turns white
	0.9-1.0	1064	Old tattoo, black prison blue, operate until the tattoo turns white
	0.9-1.0	532	Wash the color and work until the tattoo turns white
Blackhead	1.1-1.3	1064	Knock the little black head off

Taboo group

1, pregnant women hypertension heart disease diabetes;

2, people who are allergic to light are prohibited;

3. People with open wounds;

4. People who cannot avoid private life in the near future;

5. Prohibited during menstruation.

Instructions

Precautions after treatment

1. Ice
Usually the skin will be slightly red after treatment, similar to the feeling after the sun, you can use an ice pack on the treated position for 15-30 minutes.
2, strengthen moisturizing within a week after the skin will produce dandruff or scab, please strengthen moisturizing repair (can rub moisturizing essence), and do a good job of sun protection, and try to avoid makeup (will make the skin dry), the scab will slowly fall off in 3-5 days.
3, when operating eyebrows, there can be no water below, keep dry.
4, if there is a phosphor check, it is recommended to repair first, and then do the piosecond, such as directly do easy return melanin, because the previous pigment is forcibly suppressed by harmful substances isolated.
5, the operation of energy, according to the local weather, ultraviolet light, the adjustment of energy is different.
6, if there is a need to eat Chinese medicine every other week to operate.

Note:
The machine is a light product. During operation, be careful not to point at people's eyes. After operation, you need to put the handle into the protective cover to prevent misoperation from hurting people.