Enhances Contours / Tightens Skin / Eliminates Sagging

Vertical EMface

Instrument Manual



Catalogue

Product introduction

Working principle 01

Product specifications 01

Structure introduction 02

Instructions for use

Interface instructions 04

Parameter setting 09

Warning 09

Precautions 10

Configuration list 10

Product introduction

EMFace

EMFace is a device that can deliver energy to the muscle layer. As we age, the loss of muscle tissue leads to facial sagging, reduced fullness, insufficient facial support, and sunken skin. EMface can effectively solve above problems. Especially when the cheek muscle begin to sag, EMface can strengthen lifting muscles and provide deeper support. And then perform fascia lifting (HIFU) and dermis lifting (RF such as Thermage, or photoelectric project)can get twice the result with half the effort. If you want to fight against severe sagging, you must have multi-dimensional and multi-level skin maintainance.

Working principle


EMFace working principle： RF and the proprietary HIFES™ technology. HIFES™ is also called high-intensity focused electromagnetic field, which is specially designed to stimulate facial muscles. RF heats skin tissue to stimulate collagen production, thereby improving skin texture and elasticity， The HIFES™ technology achieves tissue remodeling by stimulating deep facial muscles and collagen, effectively improving the aging caused by the loss of facial muscle tissue.

Product specifications

EMFace specifications	
screen pixels	1080x1920
Theory	RF + HIFESTM
Electromagnetic Energy	0-3.8T
RF	1MHz
Pulse width	200us
Package Size	62*48*114CM
Pulse Shape	Biphase Wave
GW	58.15KG

Product introduction

Structure introduction

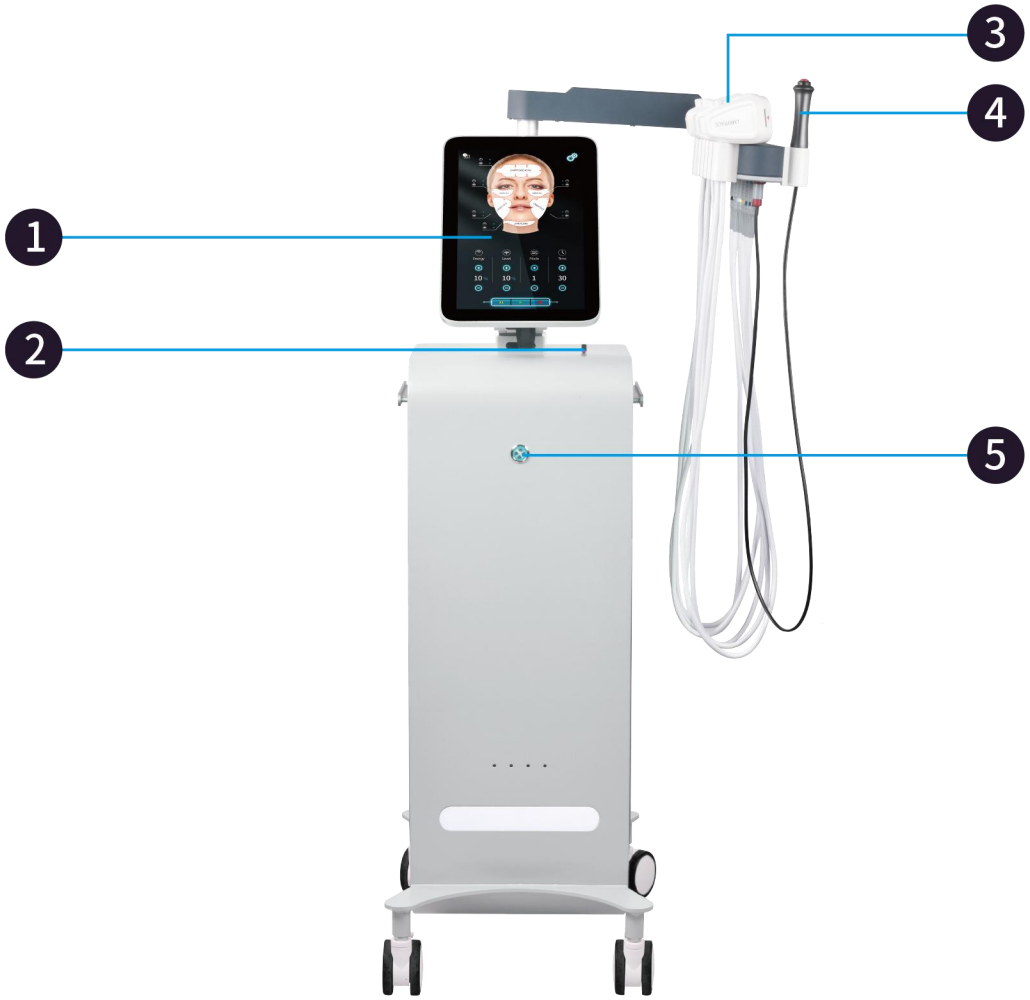

Product Front

(The picture is subject to the actual object)

1 Super Clear Touch screen 2 USB Socket 3 Adapter Box

4 Handheld Emergency Stop Rod 5 On/Off button

Product introduction

Structure introduction




Product Back

(The picture is subject to the actual object)


1. Power Switch
2. Power Cable Socket
3. Emergency Stop Rod Plug
4. A1,A2,B1,B2,C1,C2 Plug

Instructions for use

Interface instructions

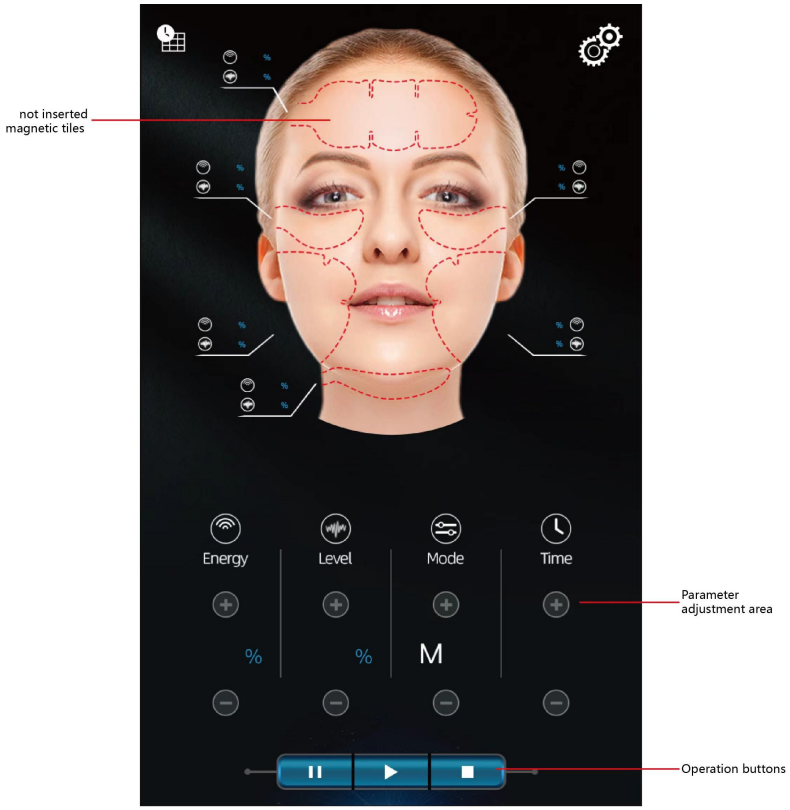

(1-1)

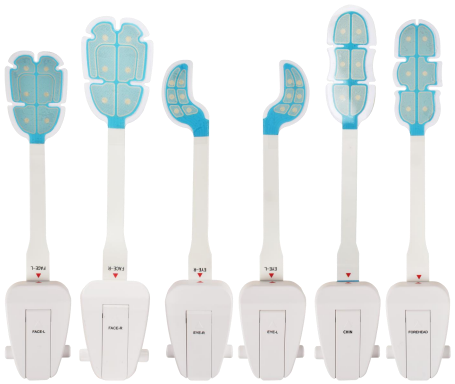


(1-2)

Before operation, first connect the Face USB (black USB) to the instrument, then turn on machine. The interface shown in picture (1-1) will appear. The interface shows that the magnetic tile is not connected. Please connect the magnetic tiles and corresponding adapter box , as shown in the figure (1-2).

Instructions for use

Interface instructions

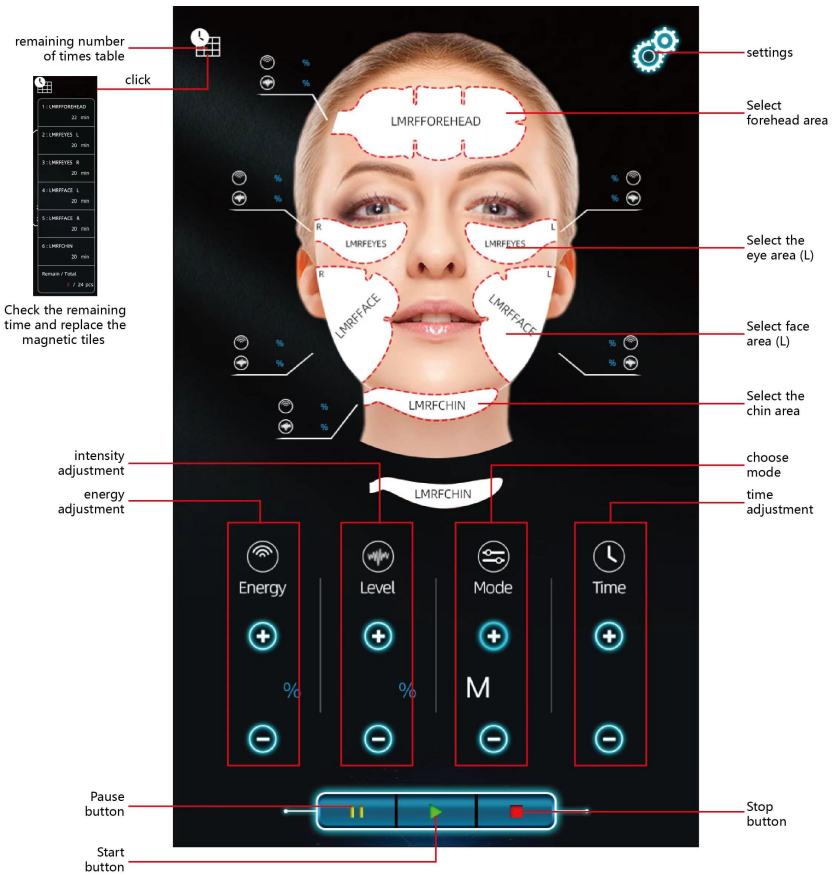

(1-3)


1、Please connect the face magnetic tiles to corresponding adapter box, as shown in picture （1-3）， If an Installation error occurs, there will be a prompt on the screen and it needs to reinstall.

2、After applying the body magnetic tiles to the area to be treated, adjust the energy, intensity, mode and time. At the beginning, adjust the energy from the lowest level. After two minutes of adaptation, increase the energy intensity.

3、When adjusting energy and intensity, you need to first click on the corresponding magnetic tiles you want to adjust on the screen, then increase or reduce the energy and intensity.（For example, if you click chin magnetic tiles, it will appear above the parameter adjustment area， then you can adjust the parameters of it.）；

4、The energy in the forehead area should be smaller than that in other parts, and the operation time is recommended to be 20 minutes.。

Interface instructions

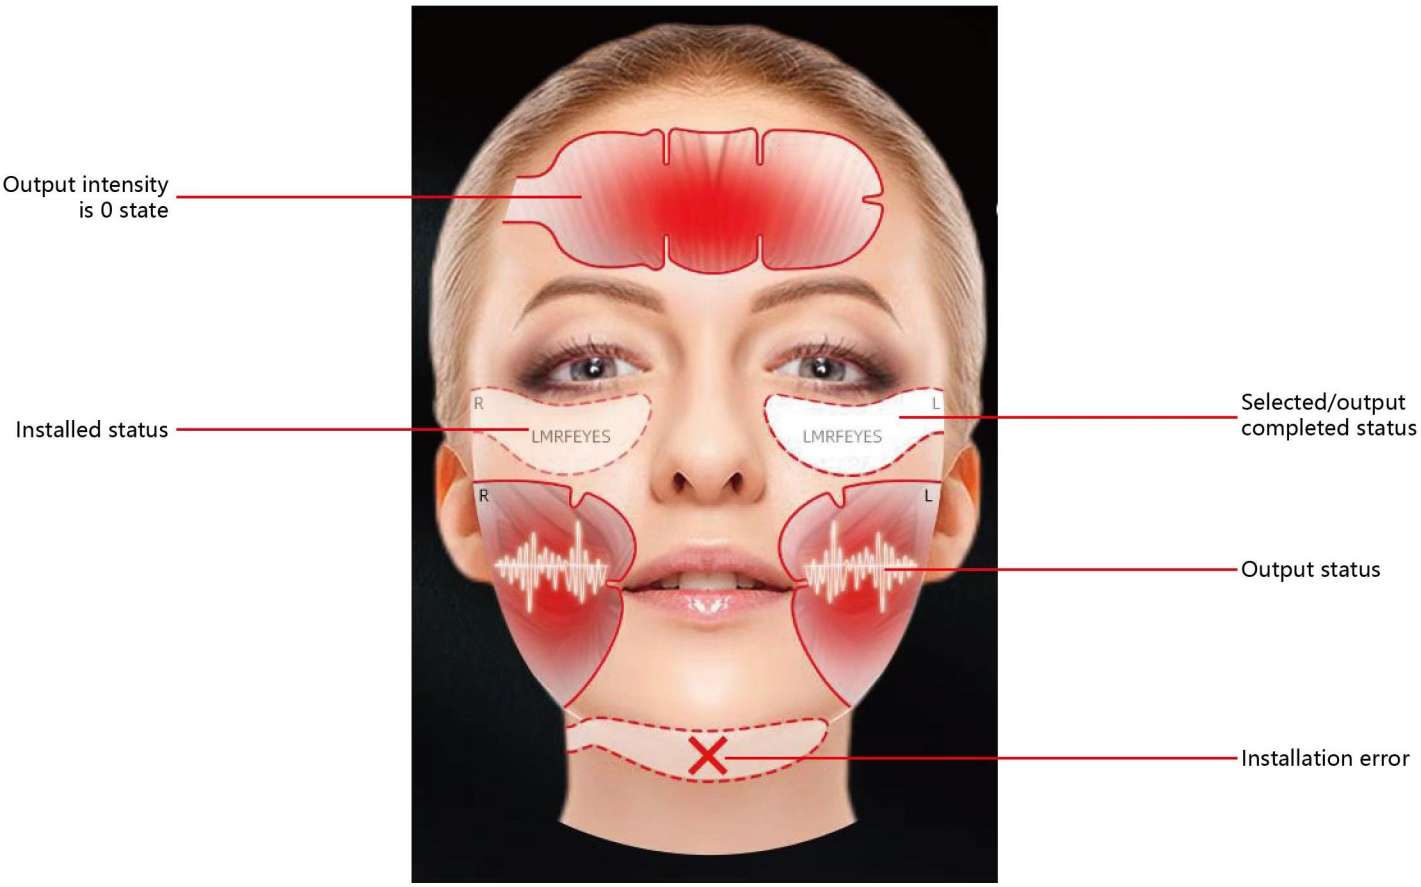


(1-4)

When the face magnetic tile is working on the face, there will be a part displayed on the screen, and the instrument will automatically stop when the operation is completed, as shown in Figure (1-4); If an Installation error occurs, there will be a prompt on the screen and it needs to reinstall.

Interface instructions



(2-1)

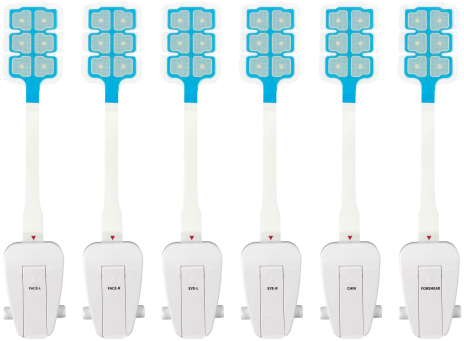


(2-2)

Picture (2-1) is the body operation interface. Before operation, first connect the body USB (red USB) to the instrument, Then turn on machine, and the interface in picture (2-1) will appear. The interface shows that the magnetic tile is not connected. Please connect the body magnetic tiles to adapter box, The magnetic tiles are identical and can be used on the same body parts, as shown in picture (2-2).。

Instructions for use

Interface instructions

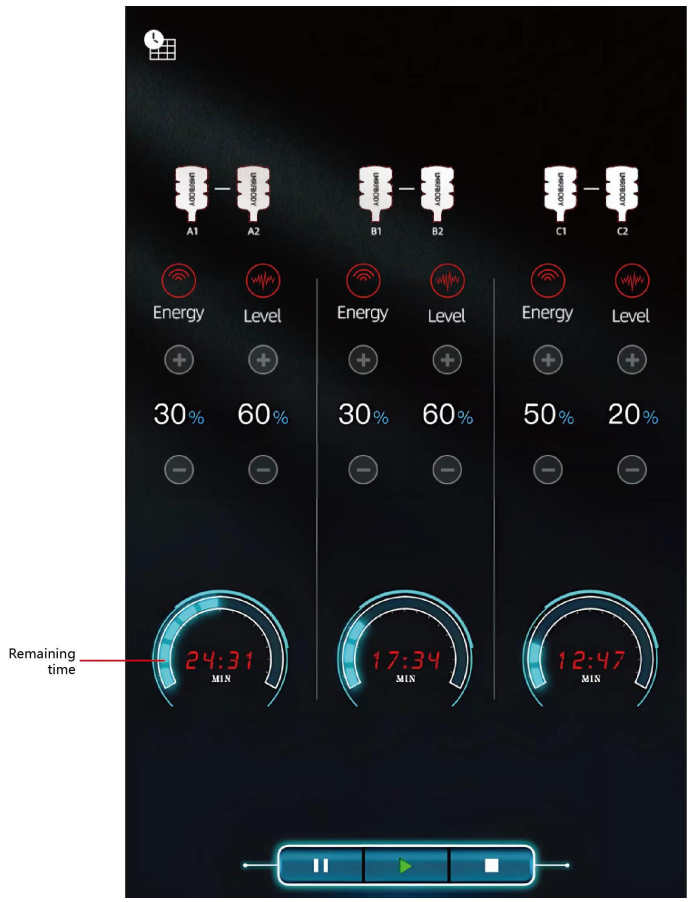

(2-3)

1、After connecting the body magnetic tiles to adapter box， as shown in picture （2-3）If an Installation error occurs, there will be a prompt on the screen and it needs to reinstall.

2、After applying the body magnetic tiles to the area to be treated, adjust the energy, intensity, mode and time. At the beginning, adjust the energy from the lowest level. After two minutes of adaptation, increase the energy intensity.

3、When adjusting energy and intensity, you need to first click on the body magnetic tiles you want to adjust on the screen, then increase or reduce the energy and intensity.

Instructions for use

Parameter setting

EMFace parameter setting

(Actual operation will be adjusted based on patient's feedback during treatment.)

MFace	Eye	Face	Forehead	Body
Energy	Start from 10%	Start from 40%	Start from 10%	Start from 40%
Time	20 minutes	30 minutes	20 minutes	30 minutes

Warning

1、Pregnant women, patients with high blood pressure, heart disease, diabetes, and hyperthyroidism;

2、Do not do this treatment within three months after facial surgery;

3、Skin areas have open wounds;

4、People who have received radioactive therapy for less than 3 months;

5、People with skin disease or skin inflammation, and people suffering from purulent acne;

6、Don't do this treatment before three hours after drinking。

7、People with numerous dental implants.

Instructions for use

Precautions

1、Do sun protection after the treatment, and use a mask every day for 3-5 consecutive days to enhance hydration.;
2、Don’t wash face with hot water within 24 hours after the treatment, only water that does not exceed body temperature. No swimming, hot springs or saunas;
3、Don’t put on heavy makeup immediately after the treatment but you can put on simple makeup;
4、When the skin is red after the treatment, you should avoid strenuous exercise and avoid sweating;
5、Treatment with other instruments should be done at least one week apart, except for basic care.

Configuration list

Item	quantity
Machine	1 pcs
Adapter Box	6 pcs
Face magnetic tiles	2 sets
body magnetic tiles	2 sets
handheld emergency stop rod bracket	1 pcs
handheld emergency stop rod	1 pcs
power cable	1 pcs

Note: Be sure to inform the customer that if they feel any discomfort during the treatment, they can immediately press the button on the handheld emergency stop rod and the instrument will stop output energy; press the button again for output when they need;